

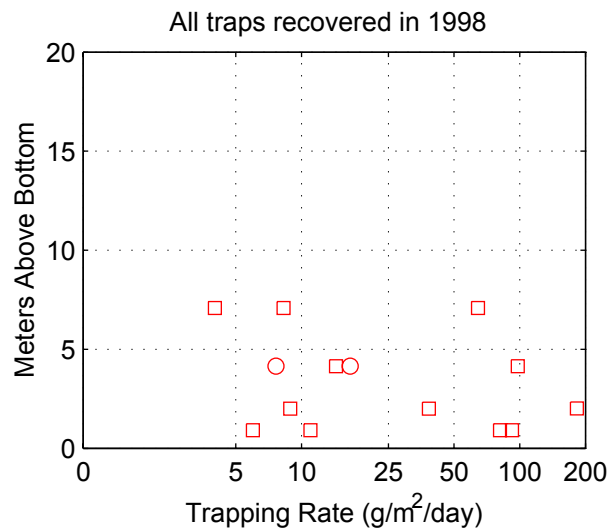
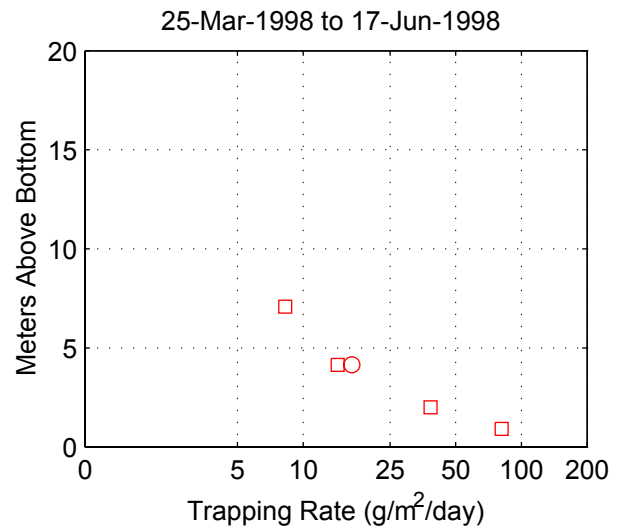
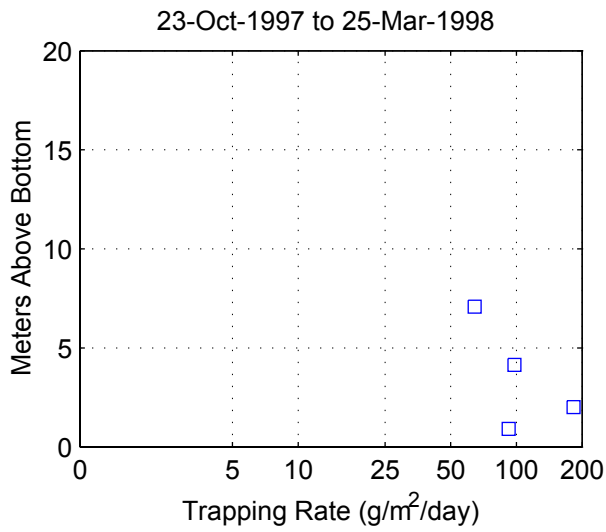
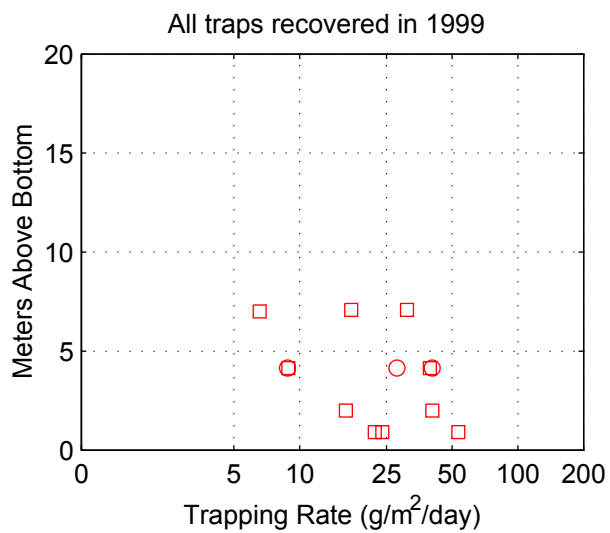


Tube Traps Recovered in 1998

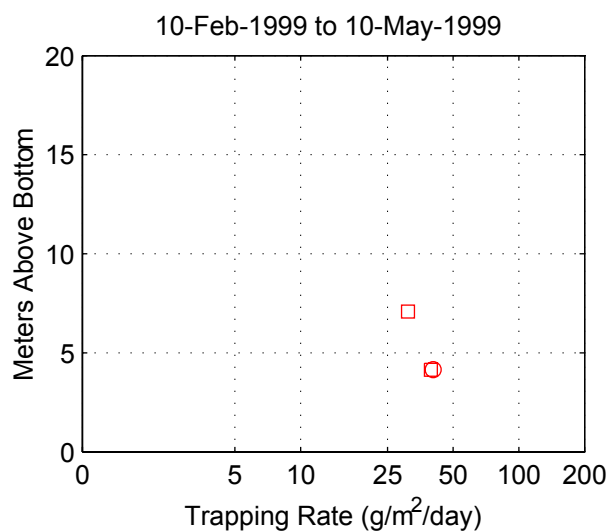




- △ Samples treated with Formalin
- Samples treated with Sodium azide
- Not treated

Tube Traps Recovered in 1999

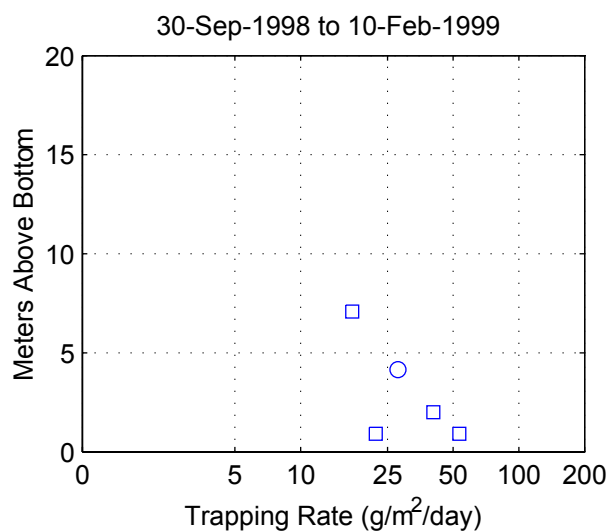

- △ Samples treated with Formalin
- Samples treated with Sodium azide
- Not treated

Tube Traps Recovered in 2000

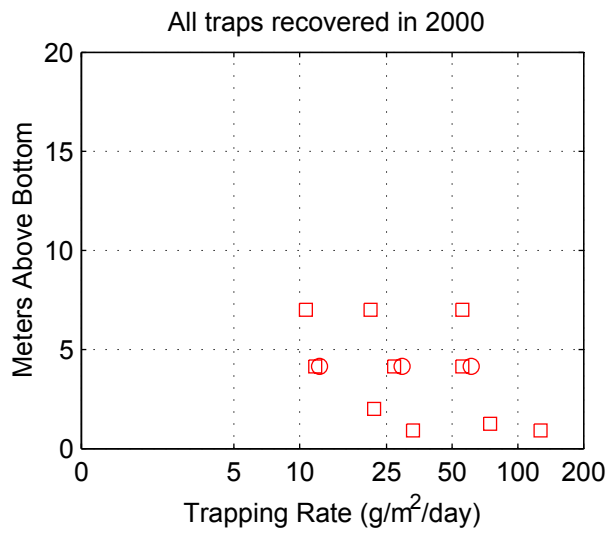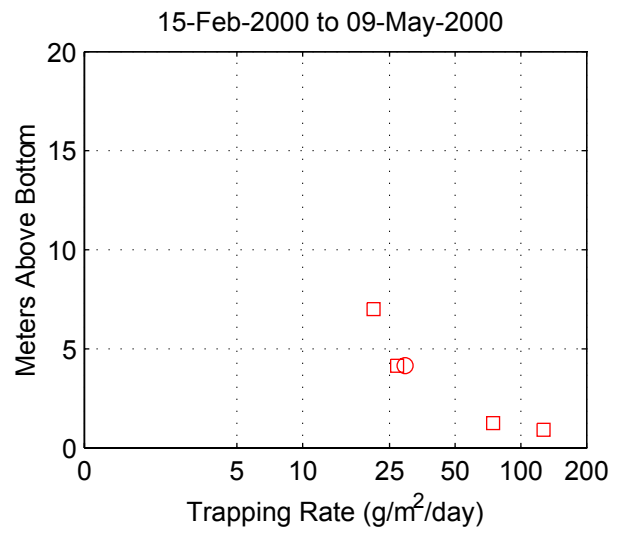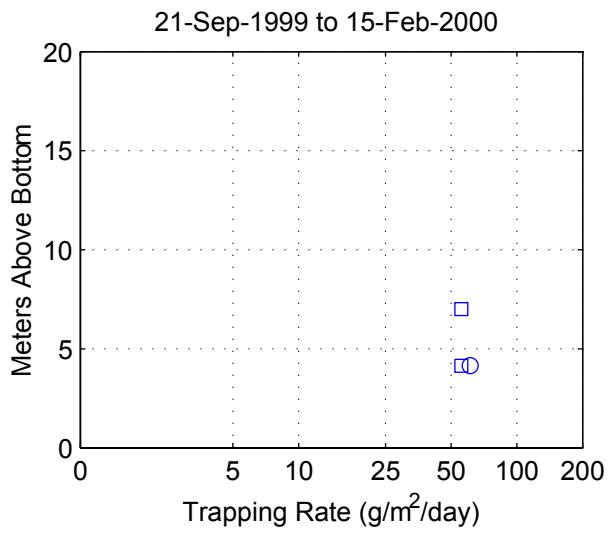

- △ Samples treated with Formalin
- Samples treated with Sodium azide
- Not treated